

1/6


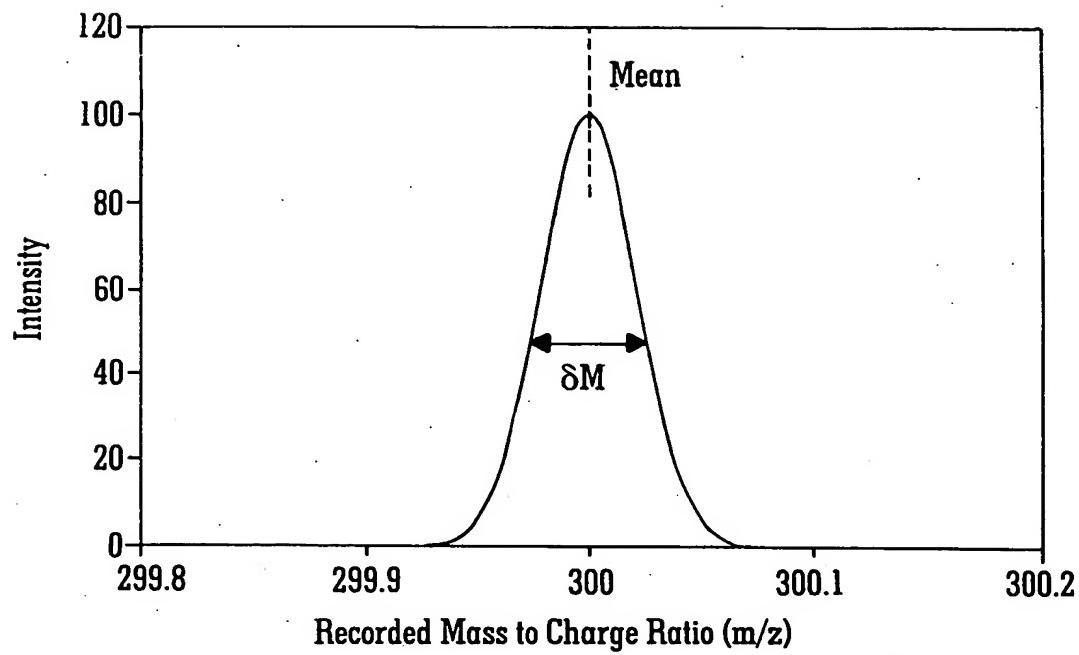


FIG. 1

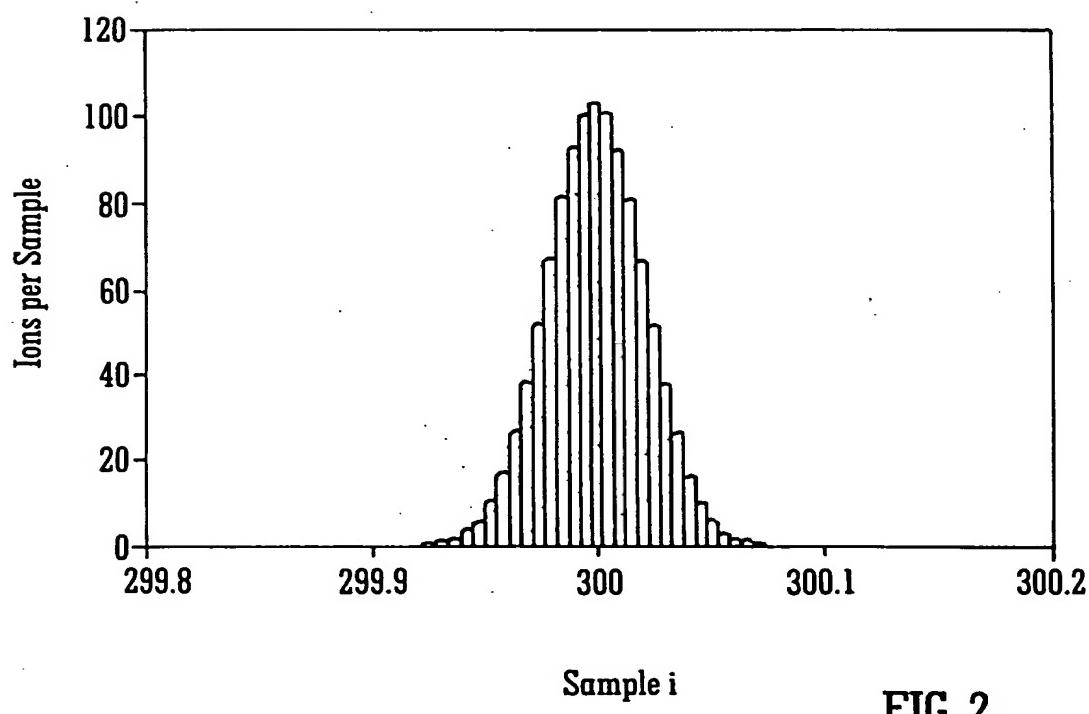

Sample i

FIG. 2

2/6

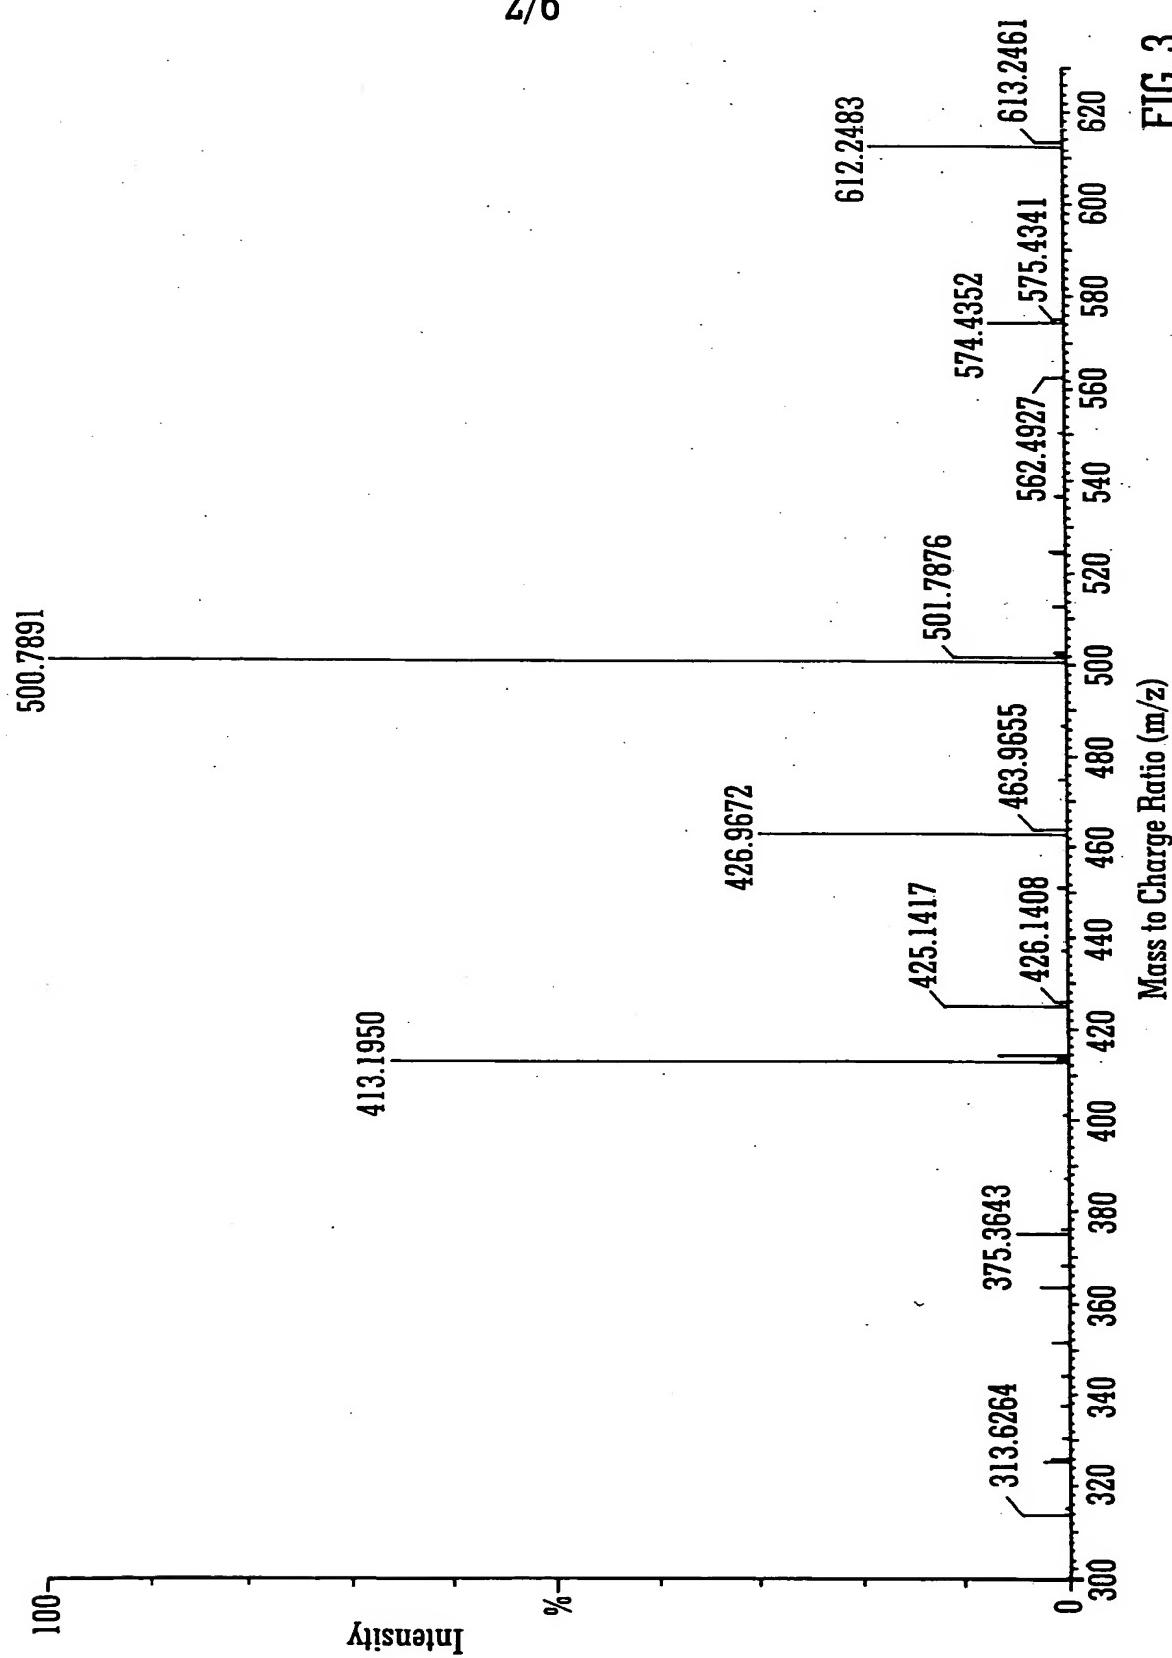


FIG. 3

3/6

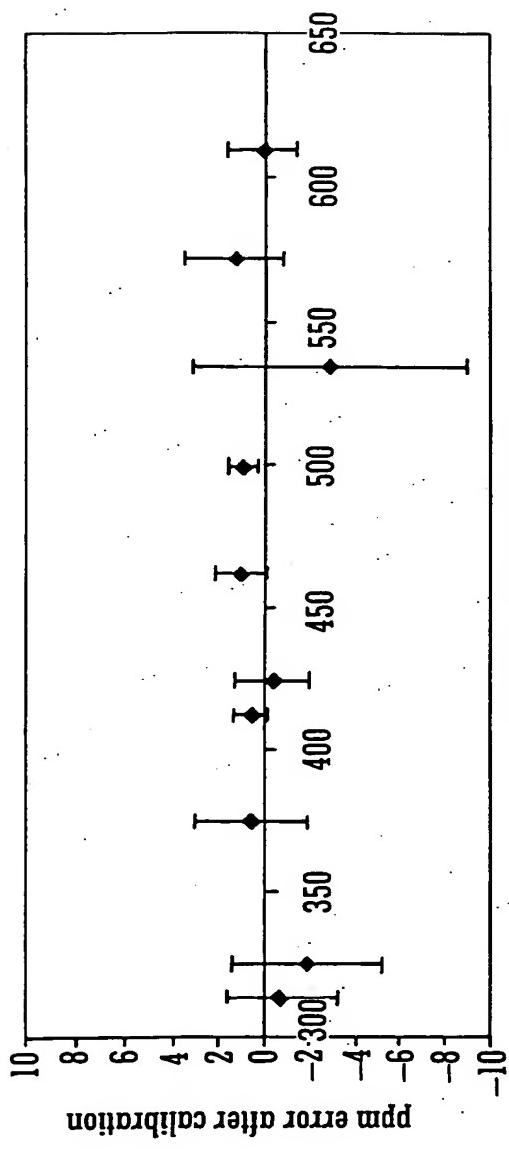


FIG. 4  
Calibration Reference  $m/z$

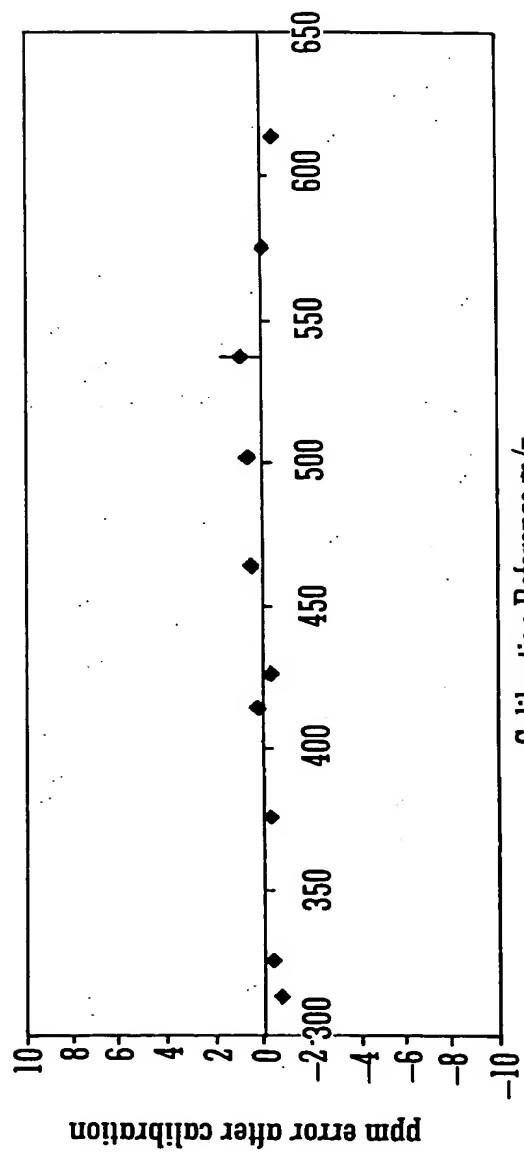


FIG. 5  
Calibration Reference  $m/z$

4/6

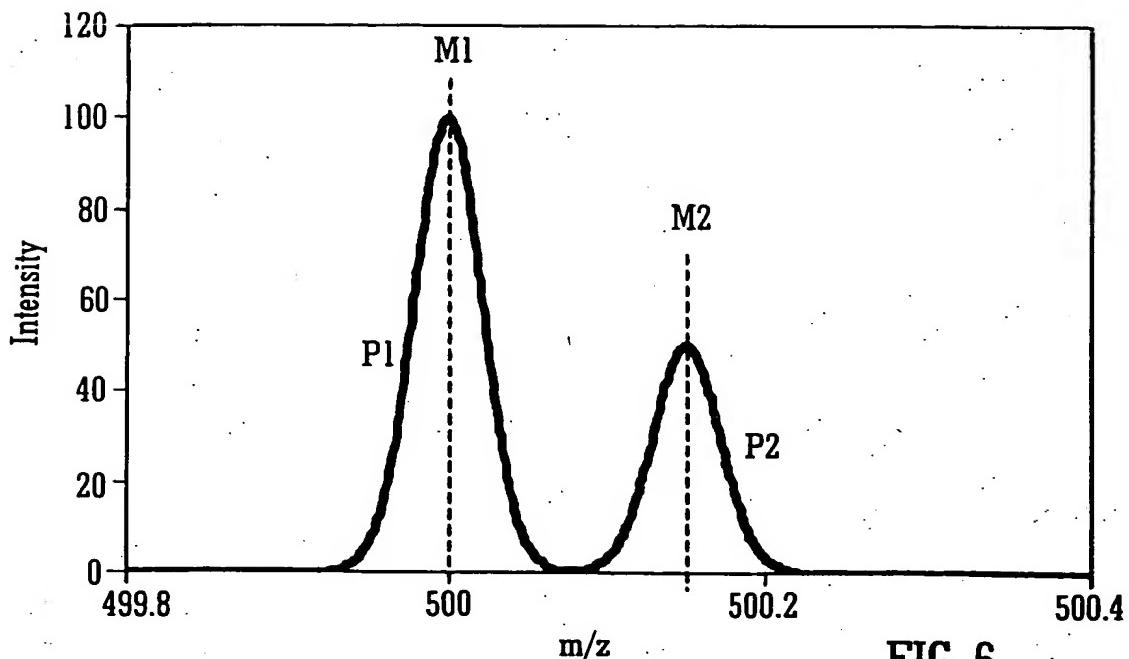


FIG. 6

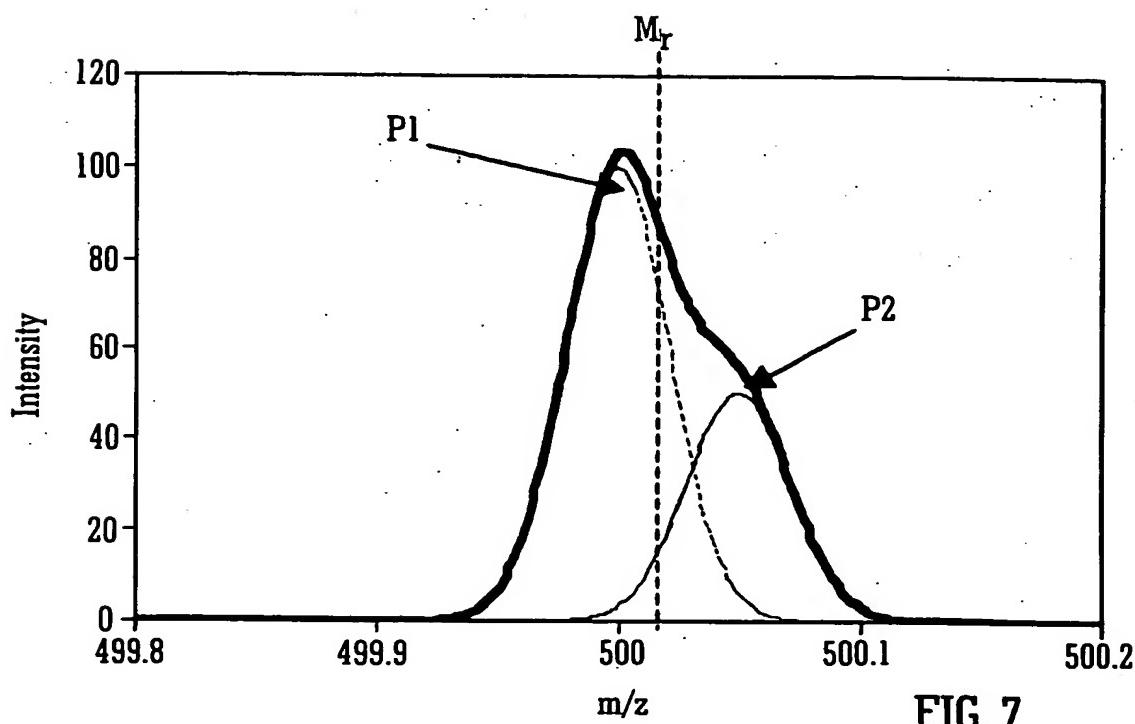


FIG. 7

5/6

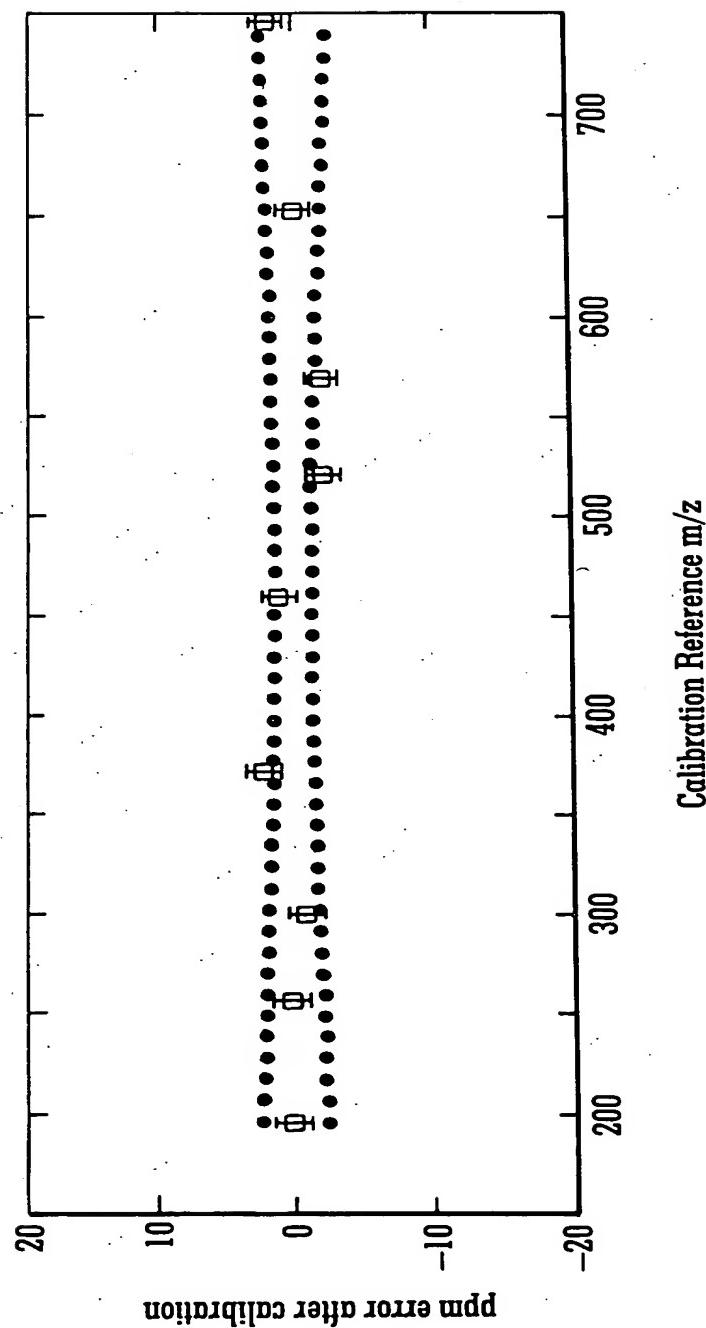


FIG. 8

6/6

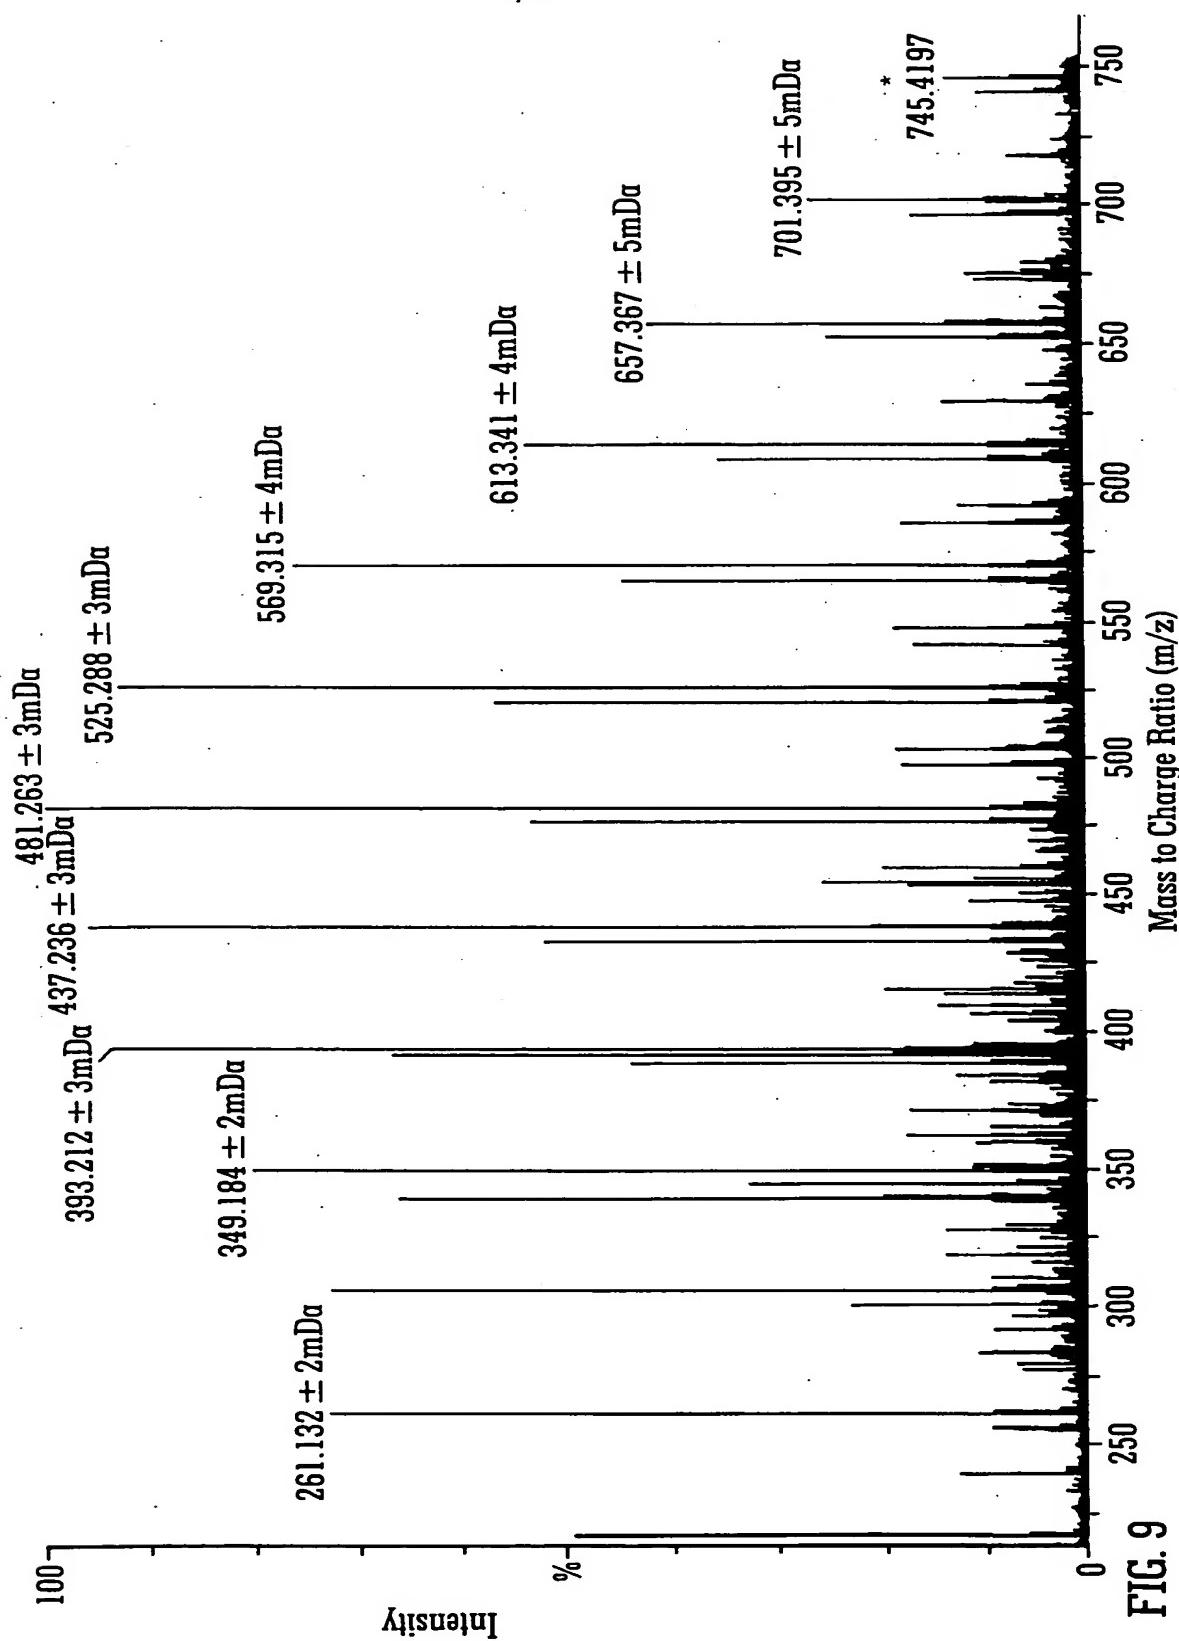


FIG. 9

BEST AVAILABLE COPY